

# DFE

Dynamic Filter Efficiency

---



[hyprofiltration.com/DFE](http://hyprofiltration.com/DFE)



# What is DFE?

## DFE matches filter testing with real-life conditions

All hydraulic and lube systems have a critical contamination tolerance level that is often defined by, but not limited to, the most sensitive system component such as servo valves or high speed journal bearings. Defining the ISO fluid cleanliness code upper limit is a function of component sensitivity, safety, system criticality and ultimately getting the most out of hydraulic and lube assets.

Filters remove the particulate contamination that enters a system or is generated by the system as it operates. All filters are subjected to some form of system dynamics: hydraulic filters encounter frequent and rapid changes in flow rate when valves shift, cylinders unload and pump output changes; lube filters experience dynamic conditions during start up and shut down. Filters validated only to current ISO testing standards don't perform as expected when subjected to the demands of real world dynamic operating systems.

A filter is not a black hole. Two key characteristics of filter performance are capture efficiency and retention efficiency. Capture efficiency can be thought of simply as how effectively a filter captures particles while retention efficiency is a measure of how effectively that filter retains the particles it has captured. A filter is not a black hole, and its performance must not be based solely on how efficiently it captures particles. If not properly designed and applied, a filter can become one of the most damaging sources of contamination in a system if it releases previously captured particles when challenged with dynamic conditions.

The Dynamic Filter Efficiency Test (DFE) is the evolution of standard hydraulic and lube filter performance testing. DFE goes further than current industry standards to quantify capture and retention efficiency in real time by inducing dynamic duty cycles, measuring real-time performance during dynamic changes and the filters ability to retain particles. DFE testing is the method for predicting worst case fluid cleanliness along with average fluid cleanliness. The DFE test method was pioneered in 1998 during a joint effort between Scientific Services Inc (SSI) and Hy-Pro Filtration.




# Dynamic Filter Efficiency

## Current Filter Performance Testing Methods

To understand the need for DFE it is important to understand how filters are currently tested and validated. Manufacturers use the industry standard ISO16889 multi-pass test to rate filter efficiency and dirt holding capacity of filter elements under ideal lab conditions.

Figure 1 depicts the test circuit where hydraulic fluid is circulated at a constant flow rate in a closed loop system with on-line particle counters before and after the test filter. Contaminated fluid is added to the system at a constant rate. Small amounts of fluid are removed before and after the filter for particle counting to calculate the filter efficiency (capture). The capture efficiency is expressed as the Filtration Ratio (Beta) which is the relationship between the number of particles greater than and equal to a specified size ( $X_{\mu_{[c]}}$ ) counted before and after the filter. In real world terms this test is the equivalent of testing a filter in an off-line kidney loop rather than replicating an actual hydraulic or lube system. It's basically a filter cart test.

Figure 1: ISO16889 Multi-Pass Test

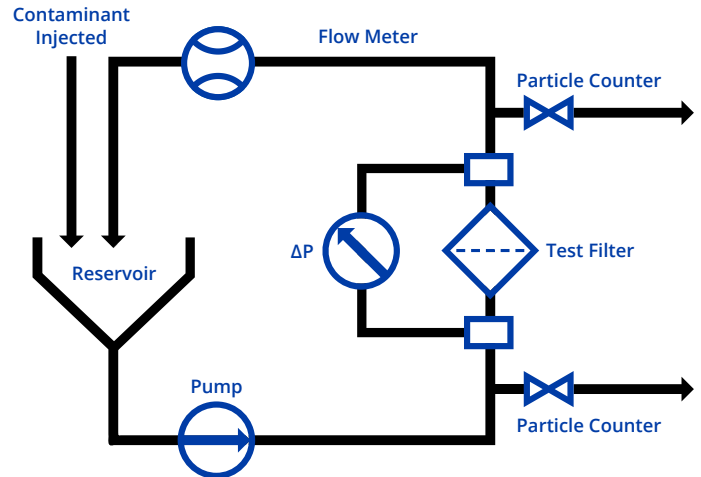

## Filtration Ratio (Beta) per ISO16889:

$$\beta_{X_{[c]}} = \frac{\text{quantity particles} \geq X_{\mu_{[c]}} \text{ upstream of filter}}{\text{quantity particles} \geq X_{\mu_{[c]}} \text{ downstream of filter}}$$

**Example:**  $\beta_{7_{[c]}} = 600/4 = 150$

**Filtration Ratio (Beta):**  $\beta_{7_{[c]}} = 150$

In the example, 600 particles greater than or equal to  $7\mu_{[c]}$  were counted upstream of the filter and 4 were counted downstream. This Filtration Ratio is expressed as "Beta  $7_{[c]} = 150$ ". The  $_{[c]}$  is referred to as "sub c". The sub c is used to differentiate between multi-pass tests run per the current ISO16889 multi-pass test with new particle counter calibration per ISO11171 from ISO4572. Filtration Ratio expressed or written without the "sub c" refers to the antiquated ISO4572 multi-pass test superseded by ISO16889. The efficiency may also be expressed as a percentage by converting the Filtration Ratio:

$$\text{Efficiency of } \beta_{X_{[c]}} = \frac{(\beta-1)}{\beta} \times 100$$

**Example:** **Efficiency % of  $\beta_{7_{[c]}}=150 = (150-1)/150 \times 100$**

**Efficiency %:** **99.33%**

Using our Beta Ratio found in the first example, we can calculate that the test filter is 99.33% efficient at capturing particles  $7\mu_{[c]}$  and larger.

# Dynamic Filter Efficiency

## The DFE Multi-Pass Testing Method

DFE multi-pass enhances the industry standard by inducing dynamic conditions (duty cycle) and measuring the effects of the duty cycle in real time instead of looking at normalized numbers over a time weighted average. DFE also quantifies retention efficiency in real time in order to identify a filter's ability to properly retain previously captured contaminant and the degree to which it unloads captured contaminant back into the system. For an easy comparison, think of it as a sneeze that releases a rush of contamination to levels that are well above the upper limit of fluid cleanliness then fades as the flow rate normalizes.

In the DFE test, flow rate is truly dynamic in that rapid changes can be made while maintaining full system flow through the test filter. The raw data is continuously collected and organized so filter efficiency can be reported for variable flow conditions including time weighted averages and isolated moments to reveal true filter performance during hydraulic stress conditions – exactly when you need the filter to perform at its best.

At the end of the initial test when the filter element is loaded with contaminant, it is subjected to a restart test in which the flow goes from zero to max flow in milliseconds, replicating a hydraulic or lube system restart. Through rapid particle counting with precise control, this dynamic flow change allows Hy-Pro to analyze the amount of particles released and understand both the capture and retention efficiencies of each and every filter tested.



# The DFE Testing Method


## Quantifying Contaminant Capture and Retention

Figure 2 compares the performance of two identical high efficiency glass media filter elements, one tested to ISO16889 multi-pass and the other to the DFE multi-pass method. The graph expresses the actual number of particles  $6\mu_{[c]}$  and larger counted downstream of the filter element from several data points during the tests.

Filter A2 was tested at a constant flow rate and maintained a steady efficiency throughout the test. Filter A1 was cycled between max rated flow rate and half of rated flow with a duty cycle consistent with that of a hydraulic system. The downstream counts for Filter A1 varied and were highest during changes from low flow to high flow. The peaks represent counts taken during flow change and the valleys represent counts taken after each flow change. The alternating high peaks represent counts taken during changes from low flow to high flow. As the amount of contaminant captured by Filter A1 increased, the downstream counts increased most dramatically during the flow changes from low to high. Filter element A1, not properly designed to retain previously captured contaminant during dynamic system conditions, can become a dangerous source of contamination as it captures and then releases concentrated clouds of contaminated fluid.

Figure 3 shows the particle counter raw data (top-upstream, bottom-downstream) for Element A1 before a change from low flow to high flow and Figure 4 shows the particle counter data for Element A1 during a change from low flow to high flow. The downstream particle count trace during the change reveals a much higher quantity of smaller particles and larger particles that did not pass the element before the dynamic system condition. This phenomenon can best be described as “contaminant unloading”. As the filter element captures more dirt, greater amounts may be released back into the system that it is installed to protect when the element is subjected to a dynamic flow condition and change in differential pressure across the element. Unloading may also occur when the flow rate changes from high flow to low flow, represented by the alternating smaller peaks in Figure 3. The filter element typically recovers shortly after the dynamic condition, but highly contaminated clouds of fluid from contaminant unloading can cause severe component damage and unreliable system performance.

Figure 2: Particle Counts Downstream of Filter  $6\mu_{[c]}$

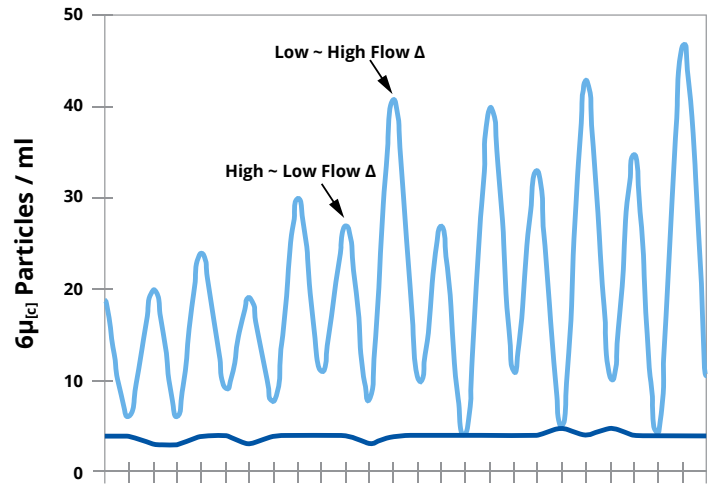

Filter Element	A1	A2
Element Rating	$\beta_{7_{[c]}} > 1000$	$\beta_{7_{[c]}} > 1000$
High Flow (lpm)	112	112
Low Flow (lpm)	56	-
Contaminant Injection Rate	3 mg/l	3 mg/l

Figure 3: Element A1 Before Flow Change


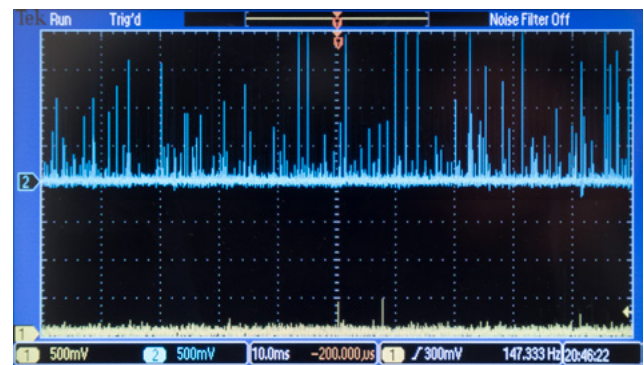


Figure 4: Element A1 During Flow Change

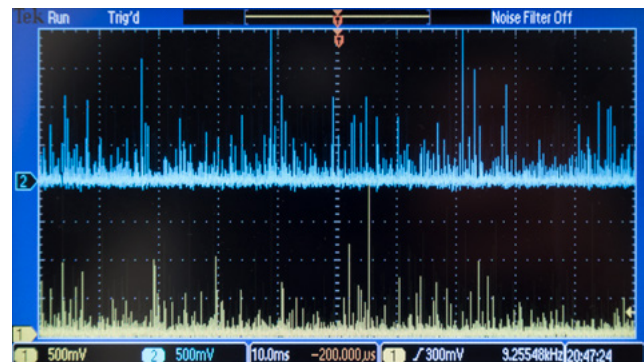


# The DFE Testing Method

## Quantifying Contaminant Capture and Retention

Figure 5 compares the performance of two identical Hy-Pro filter elements designed and developed per the DFE multi-pass test method. All Hy-Pro elements that utilize the G8 or higher media carry the Hy-Pro DFE rating.

Although the contaminant unloading effect is still evident, the unloading is insignificant as filter element Hy-Pro 1, tested per DFE, performed true to its ISO16889 multi-pass rating of  $\beta_{7_{[c]}} > 1000$  even during dynamic flow conditions.


Figure 5: Particle Counts Downstream of Filter  $6\mu_{[c]}$

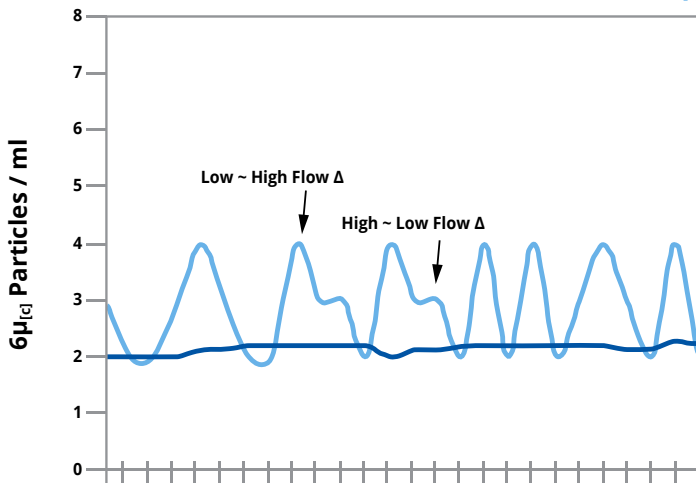

Filter Element	Hy-Pro 1	Hy-Pro 2
Element Rating	$\beta_{7_{[c]}} > 1000$	$\beta_{7_{[c]}} > 1000$
High Flow (lpm)	112	112
Low Flow (lpm)	56	-
Contaminant Injection Rate	3 mg/l	3 mg/l

Figure 6 compares the performance of filter Element A1 and Hy-Pro 1 (DFE rated). Both elements demonstrated excellent particle capture performance during the ISO16889 and DFE testing. The DFE rated Hy-Pro element yielded much more stable particle counts downstream of the element and more consistent efficiency during the dynamic flow conditions. Improving particle retention results in more predictable fluid cleanliness levels and a system that can continually operate below the ISO cleanliness code limit.

Figure 6: Particle Counts Downstream of Filter  $6\mu_{[c]}$

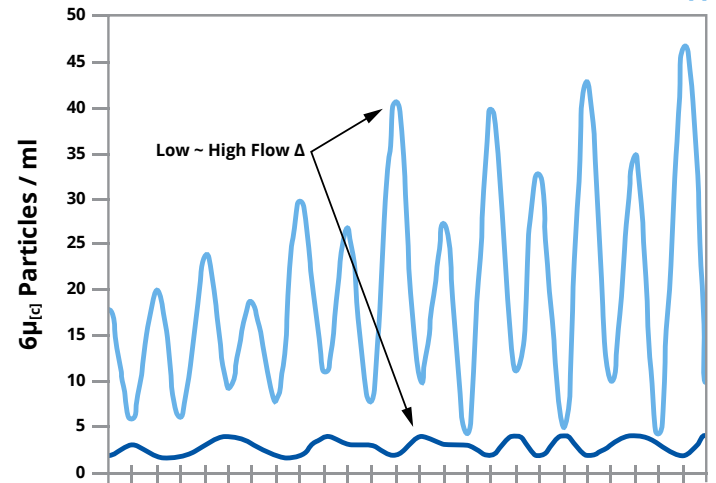

Filter Element	Element 1	Hy-Pro 1
Element Rating	$\beta_{7_{[c]}} > 1000$	$\beta_{7_{[c]}} > 1000$
High Flow (lpm)	112	112
Low Flow (lpm)	56	56
Contaminant Injection Rate	3 mg/l	3 mg/l



# The DFE Testing Method

## DFE Multi-Pass: Cold Start Contamination Retention


Once the element has captured enough contaminant to reach approximately 90% of the terminal  $\Delta P$  (dirty filter indicator setting), the main flow goes to zero and the injection system is turned off for a short dwell period. Then main flow goes to maximum element rated flow accompanied by real time particle count to measure retention efficiency of the contaminant loaded element. The dynamic duty cycle is repeated to further monitor the retention efficiency of the filter element after a restart.

Figure 7 shows the performance of an element that was subjected to the DFE restart test. During the restart, particle counts after the filter increased by a factor of 20 on the  $6\mu_{[c]}$  channel, and the ISO Codes increased by 4 codes on the  $4\mu_{[c]}$  and  $6\mu_{[c]}$  channels. During the

restart test, there is no contaminant being injected so any particles measured were released by the element or were already in the test loop. The temporary high contamination load in the fluid can pass through the sensitive components or bearings that the filter is charged with protecting if it can't retain the dirt.


Figure 8 shows the performance of a Hy-Pro element. The unloading is evident in the DFE rated Hy-Pro element, but the effect is greatly reduced. The competitor element A3 (Figure 7) unloaded 84 times more particles  $6\mu_{[c]}$  and larger than Hy-Pro, and 14 times more particles  $4\mu_{[c]}$  and larger. The DFE rated Hy-Pro element had much higher retention efficiency than the filter designed and validated only to ISO16889 multi-pass.

Figure 7: Particle Counts Downstream of Filter

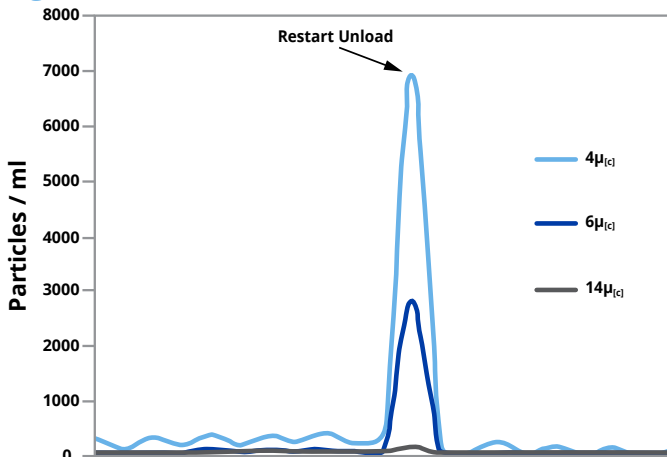

Downstream Element A3	Before Restart	During Restart
$4\mu_{[c]}$ particles/ml	429	6973
$6\mu_{[c]}$ particles/ml	136	2802
$14\mu_{[c]}$ particles/ml	25	139
ISO Code per ISO4406:1999	16/14/12	20/18/14

Figure 8: Particle Counts Downstream of Filter

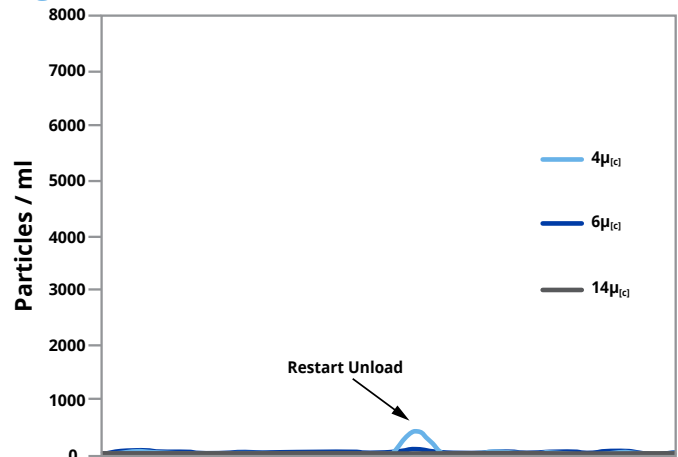

Downstream Element Hy-Pro 3	Before Restart	During Restart
$4\mu_{[c]}$ particles/ml	93	489
$6\mu_{[c]}$ particles/ml	5	33
$14\mu_{[c]}$ particles/ml	0	0
ISO Code per ISO4406:1999	14/9/0	16/12/0

# The DFE Testing Method

## DFE and ISO 16889 Multi-Pass Test Results Comparison

Figure 9 shows the performance of like elements produced by three different manufacturers that were tested to ISO 16889. The results were expressed as a time weighted beta ratio. Element B had a better capture efficiency than the Hy-Pro element in the constant flow test environment of ISO 16889. All of the elements tested were true to their Beta Ratio of  $\beta_{7_{[c]}} > 1000$ .

Figure 10 shows the time weighted performance of the like elements tested to DFE multi-pass to illustrate the performance differences between DFE and ISO16889.


In Figure 11 the particle counts taken during flow change have been isolated to measure efficiency during dynamic flow. Since the DFE test has shown that filter element performance is at its worst during flow changes, isolating those sequences can help predict performance in dynamic conditions, and it is with this graph that we see how overall filter performance changes.

Element B had a beta ratio in excess of  $\beta_{7_{[c]}} > 2000$  when tested to ISO16889 (Figure 9). However, Figure 11 shows the average beta ratio of Element B during variable flow to be  $\beta_{7_{[c]}} > 500$ . The Hy-Pro element beta ratio was in excess of  $\beta_{7_{[c]}} > 10,000$ , true to rating even in the dynamic test. The Hy-Pro performance in Figure 11 illustrates why Hy-Pro is committed to the DFE test method for design and development. DFE is Hy-Pro's competitive advantage.

Relying solely on ISO16889 to predict how filter elements will perform in a dynamic system is like taking a boat into rough seas that has never been in the water. The current industry standard test for hydraulic and lube filter performance (ISO 16889) is a good tool for predicting performance of off-line filters and circulating systems, but it does not accurately represent the stress of a hydraulic circuit with dynamic flow conditions or a lube system cold start. Without DFE testing, it is difficult to truly predict actual filter performance in a dynamic system.


**Figure 9: ISO 16889 Multi-Pass**

Time Weighted Beta Ratio Comparison for  $\beta_{7_{[c]}} > 1000$  Filter Element

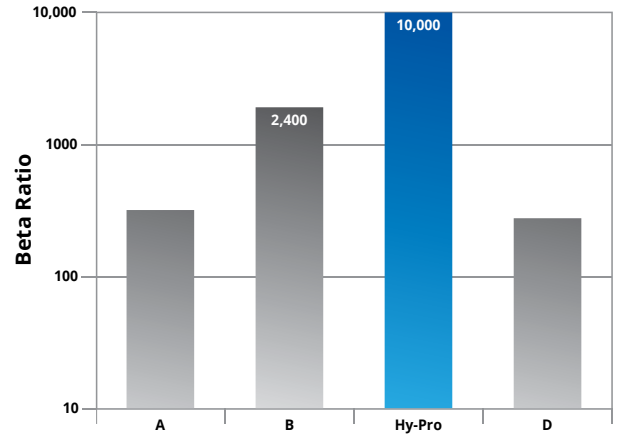


**Figure 10: DFE Multi-Pass**

Time Weighted Beta Ratio Comparison for  $\beta_{7_{[c]}} > 1000$  Filter Element

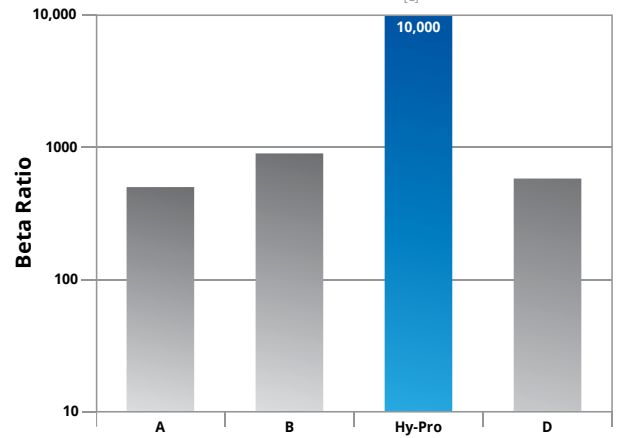

**Figure 11: Real Time Flow Change**

Beta Ratio Comparison per DFE Multi-Pass for  $\beta_{7_{[c]}} > 1000$  Filter Element

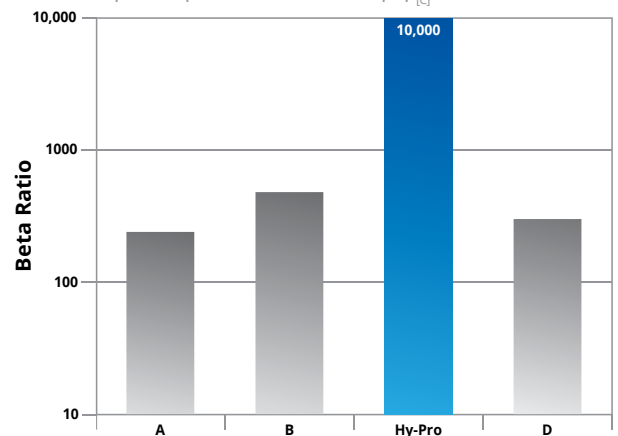

**Want to find out more? Get in touch.**

hyprofiltration.com  
info@hyprofiltration.com  
+1 317 849 3535

© 2016 Hy-Pro Corporation. All rights reserved.



MKTLIT-DFE-062916-BC